

JAY ZAGER DUTY EXPERT

Intoxilyzer - Alcohol Analyzer

Model 8000

SN 80-001145

10/14/13

04:07

Test	g/210L	Time
Air Blank	0.000	04:07
Subject Test	RGE*	04:08
Breath Volume	0.679 LITERS	
Air Blank	0.000	04:09

\*Range Exceeded

  
Operator's Signature

JAY ZAGER DUI EXPERT

Intoxilyzer - Alcohol Analyzer


Model 8000

SN 80-001146

10/14/13

04:09

Test	g/210L	Time
Air Blank	0.000	04:09
Subject Test	0.420	04:10
Breath Volume	1.203 LITERS	
Air Blank	0.000	04:11

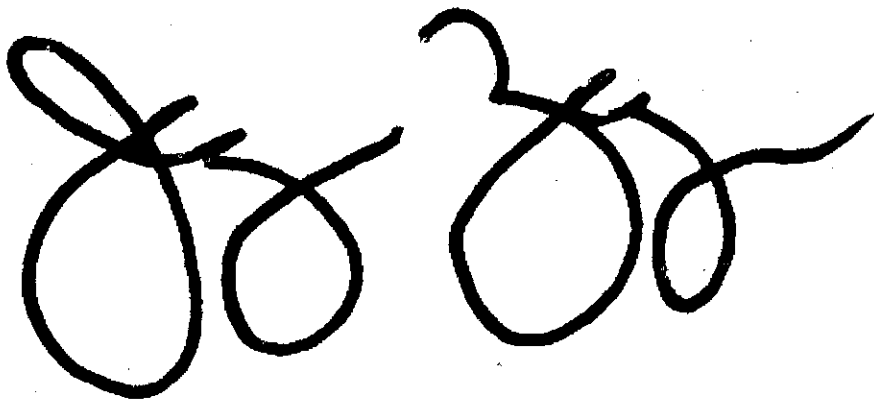A handwritten signature in black ink, consisting of two stylized, overlapping loops.

JAY ZAGER DUI EXPERT

Intoxilyzer - Alcohol Analyzer


Model 8000

SN 80-001146

10/14/13

04:11

Test	g/210L	Time
Air Blank	0.000	04:12
Subject Test	0.097	04:12
Breath Volume	2.132 LITERS	
Air Blank	0.000	04:13

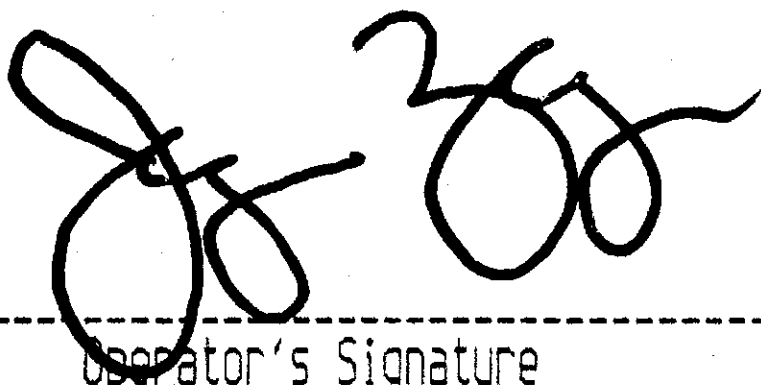

Operator's Signature

JAY ZAGER DUI EXPERT

Intoxilyzer - Alcohol Analyzer


Model 8000

SN 80-001146

10/14/13

04:13

Test	g/210L	Time
Air Blank	0.000	04:14
Subject Test	0.048	04:14
Breath Volume	2.304 LITERS	
Air Blank	0.000	04:15

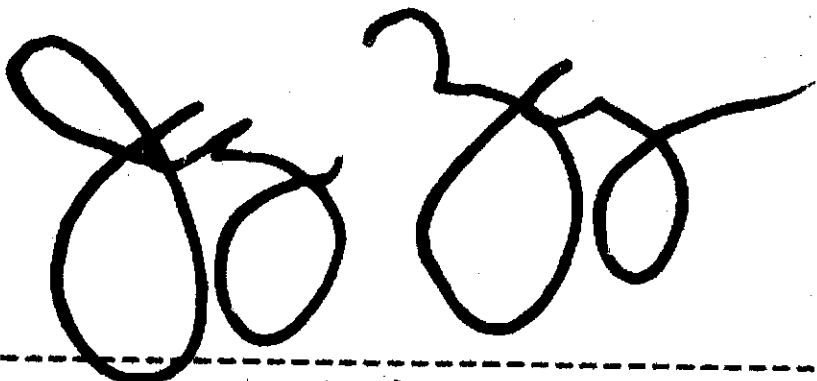

Operator's Signature

JAY ZAGER DUI EXPERT

Intoxilyzer - Alcohol Analyzer


Model 8000

SN 80-001146

10/14/13

04:15

Test	g/210L	Time
Air Blank	0.000	04:16
Subject Test	0.016	04:16
Breath Volume	1.792 LITERS	
Air Blank	0.000	04:17

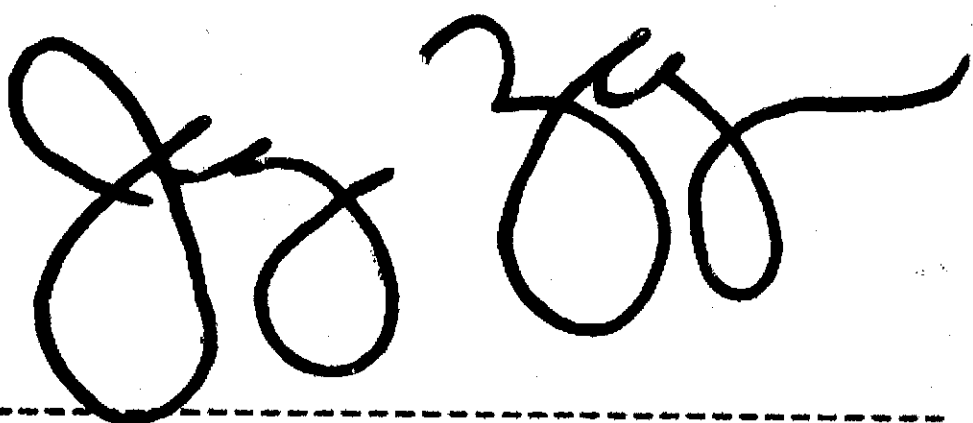

A handwritten signature in black ink, appearing to read 'Jay Zager', is written across the bottom of the page. The signature is stylized with large loops and a long horizontal tail.

JAY ZAGER DUI EXPERT

Intoxilyzer - Alcohol Analyzer

Model 8000

SN 80-001146

10/14/13

04:17

Test	g/210L	Time
Air Blank	0.000	04:17
Subject Test	0.000	04:18
Breath Volume	1.437 LITERS	
Air Blank	0.000	04:18

*Jay Zager*